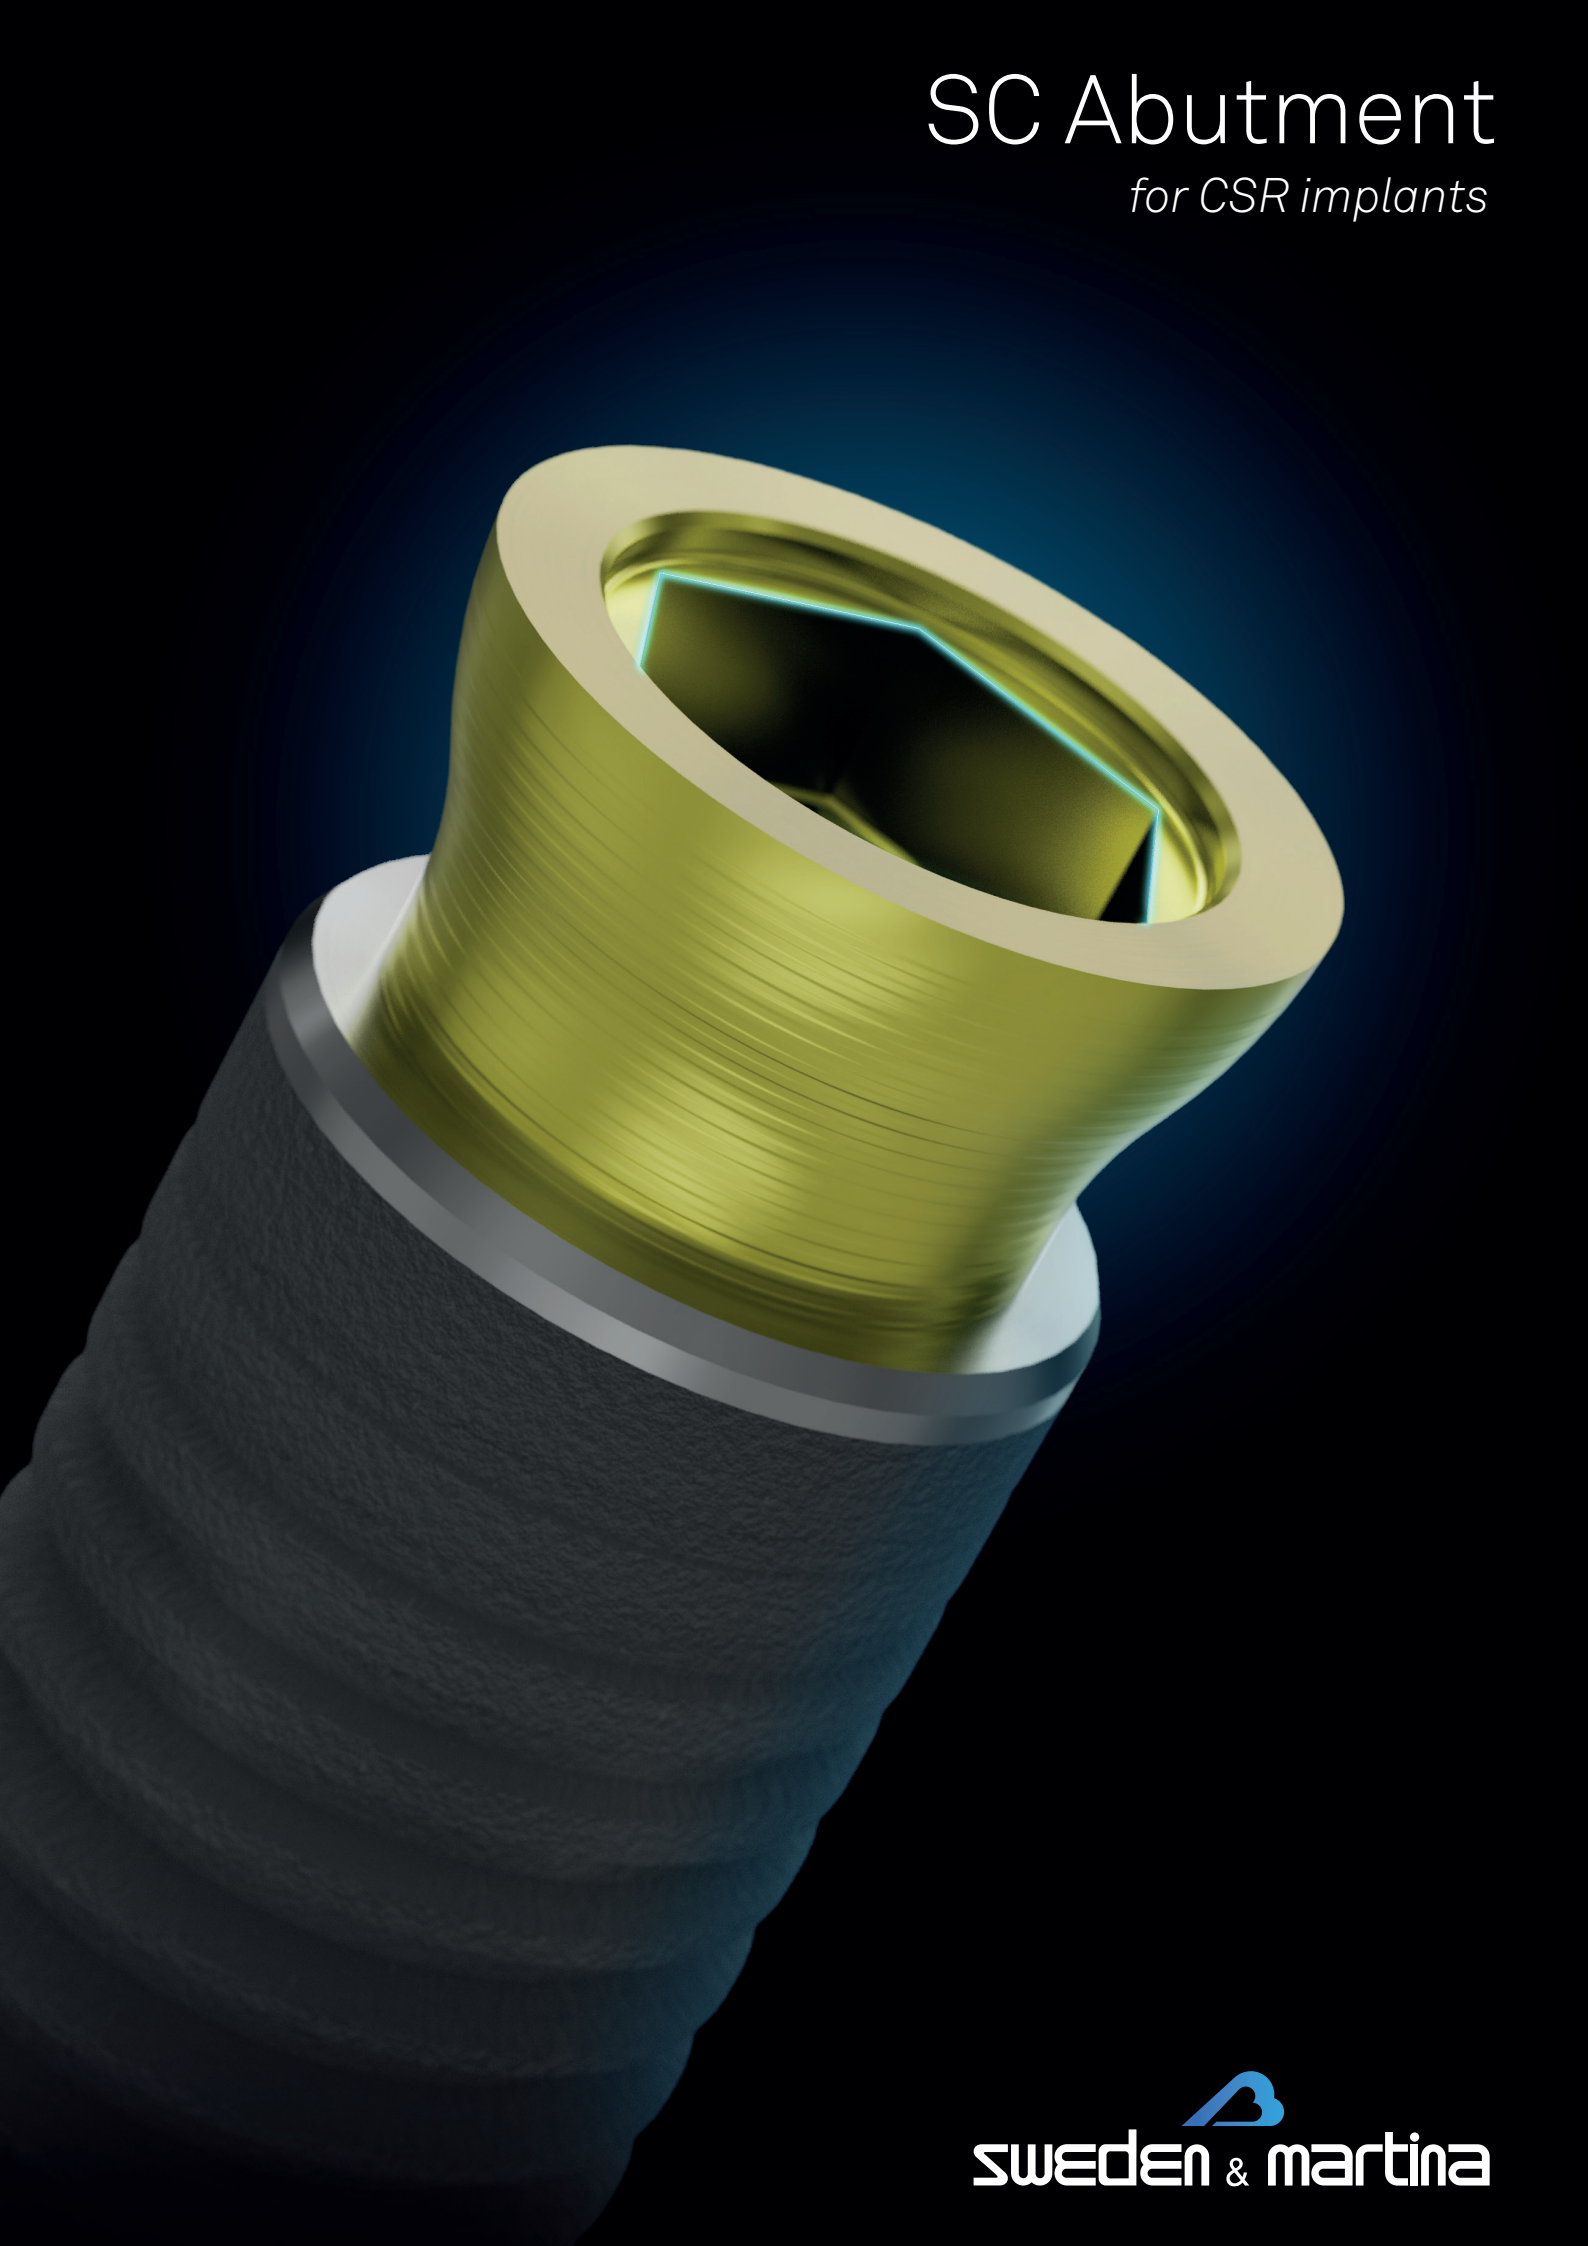
SC Abutment

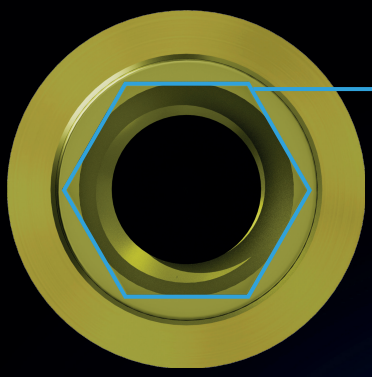
for CSR implants




sweden & martina


SC Abutments for CSR implants

Designed to create single crowns, preserving soft tissues and simplifying prosthetic rehabilitation



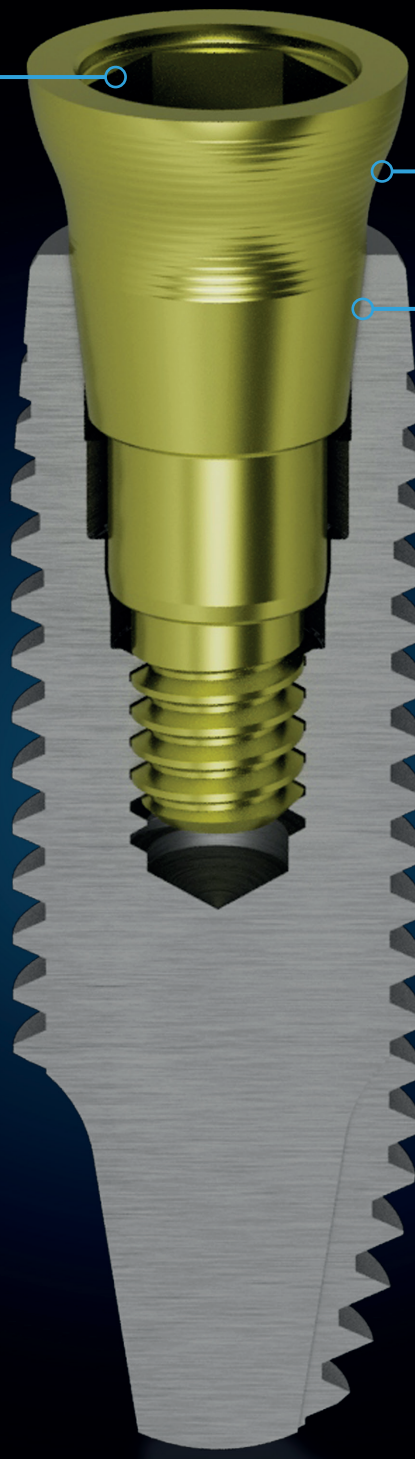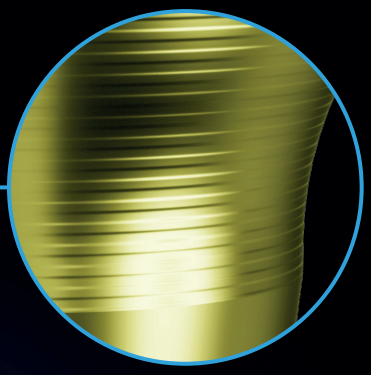Hexagonal connection for crown placement






UTM surface

The UTM surface is characterized by a **regular microcoil** that guides fibroblasts movement, promoting accelerated healing and the long-term maintenance of stable, healthy peri-implant soft tissues.




M2.0 screw

The **2.00 mm prosthetic screw** offers superior mechanical strength, **designed to withstand even the highest loads** without compromise.



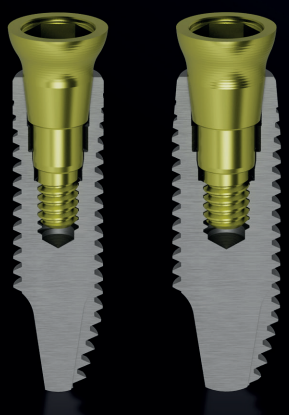The conometric fit and the absence of a screw ensure a **secure and reliable seal** against bacterial infiltration.










A single prosthetic platform for both implant connections for a simplified approach.

The abutment is **supplied with the carrier**.









SC Abutment

h mm	DAT-N Connection		DAT Connection	
2.00 mm		**VSR-PLS-N-2-ROT**		**VSR-PLS-2-ROT**
3.00 mm		**VSR-PLS-N-3-ROT**		**VSR-PLS-3-ROT**
4.00 mm		**VSR-PLS-N-4-ROT**		**VSR-PLS-4-ROT**



To tighten the abutments, use the Easy Insert with blue ring, included in the CSR kit.
The recommended torque for tightening is 25–30 Ncm.

Components for superstructures on SC abutment

straight		**PLS- CG**
L - long, straight		**PLS- CG-L**
L - long, divergent		**PLS-CGR-L**
pick-up transfer, straight emergency		**PLS-TRA***
titanium cannula, indexed		**PLS-CT****
straight post		**PLS-MD-8****

**Pick-up transfer: PLS-VTRA-200 screw included.*
*** Titanium cannula and straight post: PLS-VM-200 screw included.*

SC components for digital prosthetics

digital analog for SC abutment		**PLS-ANA-DIG***
digital titanium scanbody for SC abutment		**PLS-INT-CAMTRA-L****

**Digital analog: VADIG-180 screw included.*
***Scanbody for SC Abutment: PLS-VM-200 screw included.*

Angled-hole screw

angled-hole screw		**E-VMA-200***

Please note:*the angled-hole screw must be tightened using the dedicated screwdrivers DSPDCLH-24 and DSPDFCLH-32.*

**Angled-hole screw: to be used in combination with custom-made solutions. The libraries for EXOCAD and 3Shape can be downloaded from the Digital Atelier website.*

Standard replacement screws

prosthetic screw		**PLS-VM-200** **PLS-VM-200-10***
transfer screw		**PLS-VTRA-200**

**The prosthetic screw is also available in a 10-piece pack.*

D-B1-CSR-SC-E

rev. 07-26v.01

Sweden & Martina S.p.A.
Via Veneto, 10
35020 Due Carrare (PD), Italy
Tel. +39.049.9124300
info@sweden-martina.com
www.sweden-martina.com

Sweden & Martina Ltd
Unit 1b
Amberley Court, Whitworth Road
Crawley, West Sussex, RH11 7XL
Toll free 0800 1123575
info.uk@sweden-martina.com

Authorized Distributor
Sweden & Martina Inc.
78 John Miller Way
Unit 1021 - Kearny, New Jersey 07032
Toll free 1-844-8MARTINA (1-844-862-7846)
info.us@sweden-martina.com

www.sweden-martinainc.com

Sweden & Martina Mediterranea S.L.
España - info.es@sweden-martina.com
Sweden & Martina Lda
Portugal - info.pt@sweden-martina.com
Sweden Martina Romania srl - România
info.ro@sweden-martina.com
Sweden Martina France Sarl -France
info.fr@sweden-martina.com

The implants, prosthetic components, and surgical instruments featured in this publication are Medical Devices and are manufactured by Sweden & Martina S.p.A.
The products featured comply with ISO 9001 and ISO 13485 standards and have the CE mark in accordance with the EU Medical Devices Regulation No. 2017/745.
The Sweden & Martina facility manufactures Medical Devices in accordance with cGMP standards in effect in the U.S. and other countries around the world.

Some products may not be available in all markets.
All trademarks featured in this publication are the property of Sweden & Martina, except for products where otherwise indicated.
These products are intended for medical practices and laboratories; they are not intended for sale to patients.
Reselling, duplicating or disclosing the products contained in this publication is forbidden without the written consent of Sweden & Martina S.p.A.
For further information on the products, including indications, contraindications, warnings, precautions, and potential side effects, please refer to the Sweden & Martina S.p.A. website.
The content is current as of the date of publication. Please contact Sweden & Martina for further updates.